

1 Direct Analysis of $\delta^2\text{H}$ and $\delta^{18}\text{O}$ in Natural and Enriched Human Urine 2 Using Laser-Based, Off-Axis Integrated Cavity Output Spectroscopy

3 Elena S. F. Berman,^{*,†} Susan L. Fortson,[†] Steven P. Snaith,[†] Manish Gupta,[†] Isabelle Chery,[‡]
4 Stephane Blanc,[‡] Edward L. Melanson,[§] Peter J Thomson,[⊥] and John R. Speakman^{⊥,||}

5 [†]Los Gatos Research, 67 East Evelyn Ave, Suite 3, Mountain View California 94043, United States


6 [‡]Department of Ecology, Physiology and Ethology, Hubert Curien Multidisciplinary Institute, 23 rue Becquerel, 67087 Strasbourg
7 cedex 2, France

8 [§]Division of Endocrinology, Metabolism, and Diabetes/Division of Geriatrics, University of Colorado Anschutz Medical Campus,
9 12801 East 17th Ave, Aurora, Colorado 80045, United States

10 [⊥]Institute of Biological and Environmental Sciences, University of Aberdeen, Tillydrone Ave Aberdeen, AB24 2TZ, Scotland, U.K.

11 ^{||}State Key laboratory of Molecular and Developmental Biology, Institute of Genetics and Developmental Biology, Chinese Academy
12 of Sciences, Beijing, China

13 **ABSTRACT:** The stable isotopes of hydrogen ($\delta^2\text{H}$) and oxygen
14 ($\delta^{18}\text{O}$) in human urine are measured during studies of total energy
15 expenditure by the doubly labeled water method, measurement of total
16 body water, and measurement of insulin resistance by glucose disposal
17 among other applications. An ultrasensitive laser absorption spec-
18 trometer based on off-axis integrated cavity output spectroscopy was
19 demonstrated for simple and inexpensive measurement of stable
20 isotopes in natural isotopic abundance and isotopically enriched human
21 urine. Preparation of urine for analysis was simple and rapid
22 (approximately 25 samples per hour), requiring no decolorizing or
23 distillation steps. Analysis schemes were demonstrated to address sample-to-sample memory while still allowing analysis of 45
24 natural or 30 enriched urine samples per day. The instrument was linear over a wide range of water isotopes ($\delta^2\text{H} = -454$ to
25 $+1702$ ‰ and $\delta^{18}\text{O} = -58.3$ to $+265$ ‰). Measurements of human urine were precise to better than 0.65 ‰ 1σ for $\delta^2\text{H}$ and
26 0.09 ‰ 1σ for $\delta^{18}\text{O}$ for natural urines, 1.1 ‰ 1σ for $\delta^2\text{H}$ and 0.13 ‰ 1σ for $\delta^{18}\text{O}$ for low enriched urines, and 1.0 ‰ 1σ for $\delta^2\text{H}$
27 and 0.08 ‰ 1σ for $\delta^{18}\text{O}$ for high enriched urines. Furthermore, the accuracy of the isotope measurements of human urines was
28 verified to better than ± 0.81 ‰ in $\delta^2\text{H}$ and ± 0.13 ‰ in $\delta^{18}\text{O}$ (average deviation) against three independent isotope-ratio mass
29 spectrometry laboratories. The ability to immediately and inexpensively measure the stable isotopes of water in human urine is
30 expected to increase the number and variety of experiments which can be undertaken.

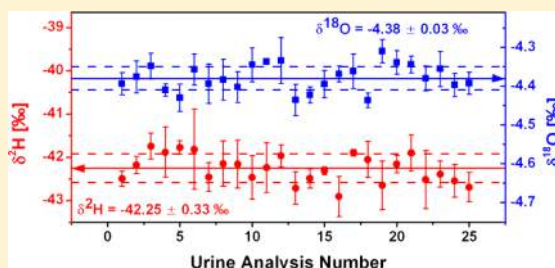

31 Analysis of the stable isotopes of hydrogen ($\delta^2\text{H}$) and oxygen
32 ($\delta^{18}\text{O}$) in human body water is used in a variety of biomedical
33 applications including measurement of total energy expenditure
34 (TEE) by the doubly labeled water (DLW) method,^{1–3}
35 measurement of total body water,⁴ and measurement of insulin
36 resistance by glucose disposal^{5,6} among other applications.
37 Currently, the vast majority of studies use isotope-ratio mass
38 spectrometry (IRMS) for analysis of $\delta^2\text{H}$ and $\delta^{18}\text{O}$ in body
39 waters. For IRMS analysis, bodily fluids (e.g., urine) require
40 either extensive purification, such as cryogenic distillation
41 followed by decolorization,⁷ or analysis by CO_2 equilibration
42 for ^{18}O measurements and zinc or chromium reduction for ^2H
43 measurements.^{8,9} These preparation methods and IRMS
44 analyses are labor-intensive, costly, and limited to only a few
45 measurement laboratories worldwide. However, in order for the
46 aforementioned biomedical applications to become widely
47 available, measurements of a large number of samples must be
48 completed quickly, accurately, and inexpensively, preferably at a
49 location near the site of sample generation.

Ultrasensitive laser absorption spectroscopy, such as off-axis
integrated cavity output spectroscopy (OA-ICOS) and cavity
ring down spectroscopy (CRDS), provides the opportunity to
measure $\delta^2\text{H}$ and $\delta^{18}\text{O}$ rapidly, accurately, and inexpen-
sively.^{10–12} Furthermore, laser-based instrumentation does
not require highly trained operators and has a small footprint,
allowing measurements to be made by researchers generating
the samples. While studies have shown that laser-based
instruments require corrections for organic contamination of
samples,^{11,13,14} two laboratories have recently shown that the
organic component of urine does not adversely affect laser-
based isotope measurements.^{7,15} O'Grady et al. utilized CRDS
to measure natural isotopic abundance human urines that had
been either cryogenically distilled or decolorized with carbon
black.⁷ Thorsen et al. used CRDS to measure natural and 64

Received: June 15, 2012

Accepted: October 18, 2012